



r25c^{PT-LITE}

FULL COMPREHENSIVE DIAGNOSTIC
COMBINED MULTIFREQUENCY MIDDLE EAR ANALYZER

PRODUCT SPECIFICATIONS



Please contact Resonance should you have any questions:
support@resonance-audiology.com

GENERAL SPECIFICATION

DIMENSIONS AND WEIGHT

- L x W x H: 370 x 290 x 180 mm
- Net weight: 3.5 kg

TEST TYPES

Tympanometry @226 and 1000Hz, Acoustic Reflex, Reflex Decay, Quick Check, Quick Screening, Multifrequency Tympanometry, Pure Tone test, Autothreshold*

DISPLAY

- 7" TFT Color display

USER INTERFACE

- Multilingual

PRINTER

- Direct printout option with selected printers

REPORTS

- .pdf report created directly from the device and stored on USB Pen drive with possibility to add patient data and tests comments via the USB Keyboard (optional)
- Data transfer to PC using Resonance Management Data Suite

"CHILDREN" FEATURE

- To help keep the child distracted while running screening "Quick Check" or "Tympanometry HF", a series of animated images appears on the color display

DATA TRANSFER TO PC

- Via cable through USB port

COMMUNICATION PORT

- Nr.1 USB host type A
- Nr.1 USB slave type B

WINDOWS® COMPATIBLE SOFTWARE

- Resonance MDS Management Data Suite

POWER

POWER SUPPLY

- 110 - 240 V AC 50/60 Hz 40 VA
- Fuses: 2 x T 1 A L 250 V


CONSUMPTION

- Max current 0.15 A
- Power consumption 40 VA

ENVIRONMENTAL

OPERATING ENVIRONMENT

- Storage: -20° C up to +50° C
- Operating: +15° C up to +35° C
- Humidity: up to 90%, (non-condensing)
- Ambient pressure: from 700 hPa up to 1060 hPa

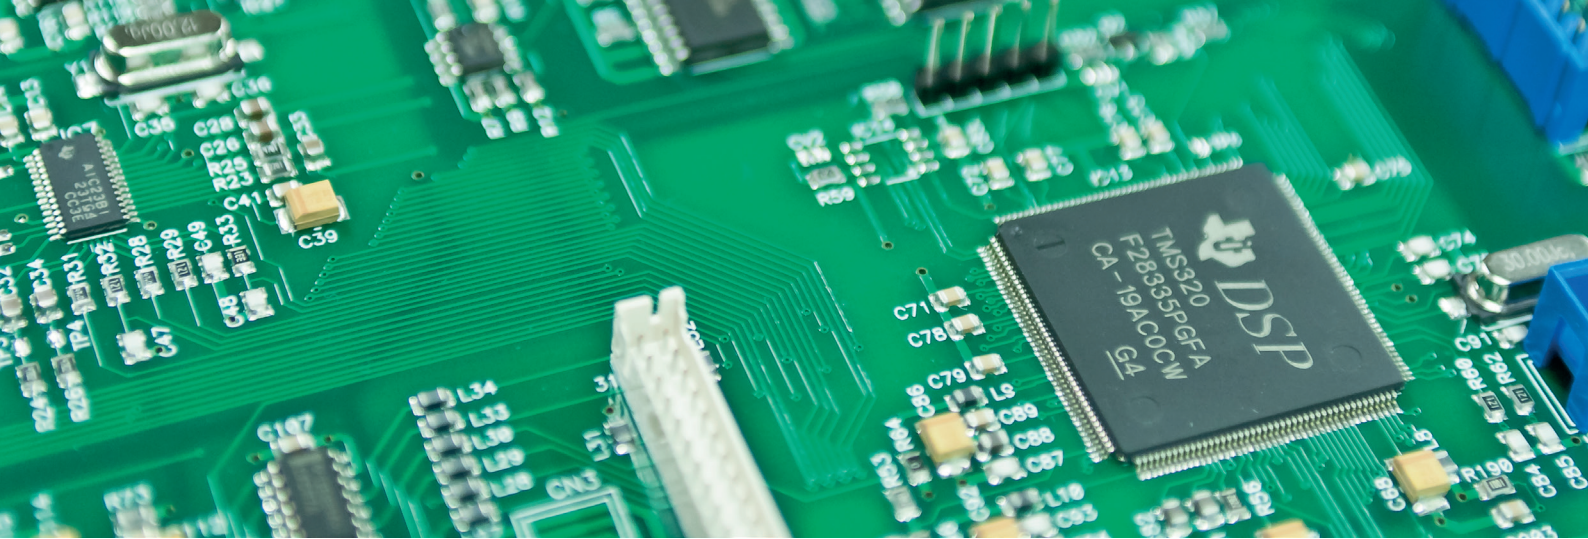

TYMPANOMETRY OPERATING SPECIFICATIONS

PROBE TONE

- 226 Hz for tympanometry
- 1000 Hz for Admittance (Y) curve tympanometry with added Susceptance (B) and Conductance (G) curves.

INTENSITY

- 226 Hz: 85 dB SPL \pm 2 dB
- 678, 800 and 1000 Hz: 75 dB SPL \pm 2 dB
- Frequency Accuracy: \pm 0.5%
- Harmonic distortion: Less than 1%

ADMITTANCE MEASUREMENTS

- Compliance range at 226 Hz: 0.05 up to 7 ml
- Sensitivity scale: Auto Scales to appropriate range, available scale at 226 Hz 1.5, 2, 5 and 7 ml
- 678, 800 and 1000 Hz: 0 to +25 mmho
- HF Sensitivity scale: Auto Scales to appropriate range, available scales for 678, 800 and 1000 Hz: 5, 10, 15, 20, 25 mmho

AIR PRESSURE

- Control: Automatic
- Range: from +200 up to -400 daPa adjustable in 50 daPa steps
- Pressure accuracy: +/- 10 daPa or +/- 10%
- Sweep rate: 50, 100, 200, 300 daPa/sec and automatic
- Indicator: Measured value is displayed
- Safety limitations: -800 up to +600 daPa

ACOUSTIC REFLEX TESTS

- Reflex test method: Threshold, Automatic, Manual
- Stimulus duration: 0.5, 1 or 2 sec.
- User selectable protocols for all test methods
- Ipsi or Contralateral stimulation for all reflex test
- Automated peak search functions available for all test methods
- Manual Reflex: Pump manual control of all stimuli
- Reflex Decay: Threshold, Automatic, Manual
- Stimulus duration: 10 or 20 sec.

FREQUENCIES AND INTENSITY RANGES

- Ipsilateral:
- Pure tone level range (dB HL) from 50 to 110
 - Noise level range (dB SPL) from 50 to 100
 - Frequency: 500, 1000, 2000, 3000, 4000 Hz
 - Noise: BBN, HP or LP
 - Accuracy: \pm 1%
 - Harmonic distortion (THD): less than 3%

Contralateral:

- Pure tone level range (dB HL) from 50 to 120
- Noise level range (dB SPL) from 50 to 115
- Frequency: 250, 500, 1000, 2000, 3000, 4000, 6000, 8000 Hz
- Noise: BBN, HP or LP
- Accuracy: \pm 1%
- Calibration accuracy \pm 3 dB
- Level steps: 1, 2, 5 or 10 dB
- On/Off ratio: 70 dB minimum

AUDIOMETRY OPERATING SPECIFICATIONS

RANGE

- Frequency range:
 - 125 - 8000 Hz (with DD45)
 - 250 - 8000 Hz (with B71W)
- Range stimuli level -10 up to 120 dB HL
- Air Conduction
- Bone Conduction -10 up to 80 dB

ACCURACY

- Frequency < 0.5%
- Distortion < 1%
- Attenuator linearity 1 dB per 5 dB step, max 3 dB whole range

TYPE OF SIGNALS

- Pure tone: sine wave 125 to 8Khz signal
- Warble: +/- 5% frequency sine wave modulated, modulation: sine wave 5 Hz
- Narrow band noise: 24 dB/oct filtered noise
- Speech noise: 1 khz 12 dB/oct filtered noise
- White noise
- External signal
- External mike
- On/Off rise - fall time: 40msec

OUTPUT TRANSDUCERS

- ACR, ACL: 10 ohm DD45 matched pair earphone
- IP30 Insert earphones (optional)
- BC: B71W Radioear
- INSERT: Insert transducer (optional)
- Free field output: 600 ohm impedance

STIMULUS PRESENTATION MODALITY

- Presentation: Normal, Reverse, Extended (present tone for 1 second from 20dB below the maximum level)
- Modality: Continuous, Pulsed (rate 0.5, 1 and 2 Hz)

QUALITY SYSTEM

Manufactured, designed, developed and marketed under an ISO 13485, ISO 9001 certified quality system. Medical CE marks and FDA approval.

COMPLIANCE/REGULATORY STANDARDS

Designed, tested and manufactured to meet the European and International Standards:

- MDD 93/42/EEC and its revised versions: Class IIa (as referred to in Annex IX, rule 10 of said MDD 93/42 EEC)
- Safety: IEC 60601-1, 3rd edition, Class 1 Type B
- EMC: IEC 60601-1-2
- Impedance: IEC 60645-5/ANSI S.3.39 Type 2
- Audiometer: to IEC 60645-1; IEC 60645-2 and ANSI S3.6, Type 2A

STANDARD ACCESSORIES

- Probe HF
- Headband and probe handle
- Probe cleaning tool kit
- DD45 for Contra
- Kit of assorted ear tips; size from 6 mm up to 15 mm
- Calibration cavity with probe holder
- Device dust cover
- Multilingual Quick user's handbook
- Pen Drive
- Resonance® MDS software with NOAH® module included (demo version)
- Power supply cable (110 - 220 V)
- Spare fuse
- DD45 headset for audiometry testing
- B71W bone conductor
- Patient response pushbutton

OPTIONALS

- Kit of assorted silicone ear tips "MS" shape size from 8 mm up to 16 mm
- External USB Keyboard
- Carrying bag
- Insert for Contra and bone conductor masking
- Pediatric Headset (AC or BC)
- Patient microphone (talk back)
- ADC Audiocups Noise reducing headset enclosures
- Goose-neck microphone
- IP30 insert earphones
- Silent cabin cables
- Free field loudspeaker
- Operator headset with microphone and speaker (talk over and monitor)
- Additional patient response pushbutton
- MDS software license

The information, pictures and specifications found in this datasheet are intended as a general guideline for customers seeking information about supplies for Resonance equipment. Resonance makes no warranty, nor assumes any legal liability or responsibility for the accuracy, typing errors or mistakes, correctness or completeness of any information in this datasheet. The information in this datasheet was correct to the best of our knowledge at the time of printing.